

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

**THIS PAGE BLANK (USPTO)**

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization  
International Bureau




(43) International Publication Date  
8 February 2001 (08.02.2001)

PCT

(10) International Publication Number  
**WO 01/08596 A1**

- (51) International Patent Classification<sup>7</sup>: **A61F 2/01** (74) Agents: **SEAGER, Glenn, M. et al.**; Crompton, Seager & Tuft, LLC, Suite 895, 331 Second Avenue South, Minneapolis, MN 55401 (US).
- (21) International Application Number: **PCT/US00/40559**
- (22) International Filing Date: **3 August 2000 (03.08.2000)** (81) Designated States (national): **CA, JP.**
- (25) Filing Language: **English** (84) Designated States (regional): **European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).**
- (26) Publication Language: **English**
- (30) Priority Data:  
09/366,192      3 August 1999 (03.08.1999)      US  
Published:  
— With international search report.  
— Before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments.
- (71) Applicant: **SCIMED LIFE SYSTEMS, INC.** [US/US];  
One SciMed Place, Maple Grove, MN 55331-1566 (US).
- (72) Inventor: **TSUGITA, Ross, S.**; 1653 Gretel Lane, Mountain View, CA 94040 (US).
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: **GUIDED FILTER WITH SUPPORT WIRE AND METHODS OF USE**

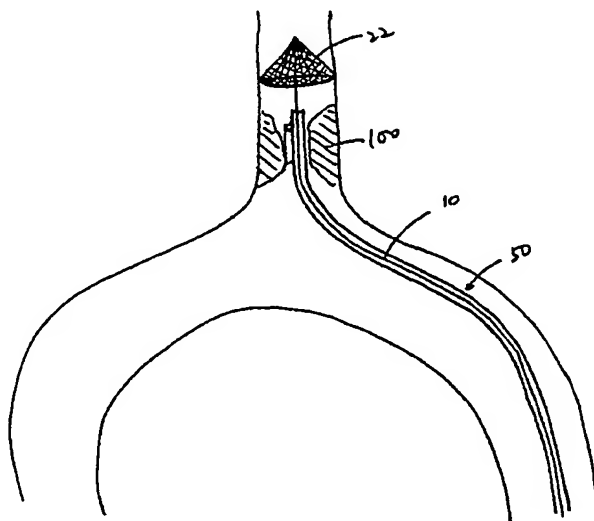

(57) Abstract: A guided filter system for temporary placement of a filter in an artery or vein is disclosed. The system includes a guidewire slideable through a wire guide included in a distal region of a support wire. The support wire has an expandable filter, which is operable between a collapsed or enlarged condition. A variety of endovascular devices, including angioplasty, atherectomy, and stent-deployment catheters, are insertable over the guidewire and/or the support wire. Methods of using the guided filter system to direct and exchange endovascular devices to a region of interest, and to entrap and remove embolic material from the vessel are also disclosed.

WO 01/08596 A1

## S P E C I F I C A T I O N

## GUIDED FILTER WITH SUPPORT WIRE AND METHODS OF USE

Field of the Invention

5                   The present invention relates generally to devices and methods for providing temporary placement of a filter in a blood vessel. More particularly, the invention provides a guidewire system for entrapment of embolic material in an artery or vein during an endovascular procedure. The system also provides a support wire for directing and/or exchanging other "over the wire" devices, such as angioplasty, atherectomy, or stent deployment catheters, to a region of interest within the vessel.

10

Background of the Invention

                  Treatment of thrombotic or atherosclerotic lesions in blood vessels using an endovascular approach has recently proven to be an effective and reliable alternative to surgical intervention in selected patients. For example, directional atherectomy and percutaneous transluminal coronary angioplasty (PTCA) with or without stent deployment are useful in treating patients with coronary occlusion. Atherectomy physically removes plaque by cutting, pulverizing, or shaving in atherosclerotic arteries using a catheter-deliverable endarterectomy device. Angioplasty enlarges the luminal diameter of a stenotic vessel by exerting mechanical force on the vascular walls. In addition to using angioplasty, stenting, and/or atherectomy on the coronary vasculature, these endovascular techniques have also proven useful in treating other vascular lesions

15

20

in, for example, carotid artery stenosis, peripheral arterial occlusive disease (especially the aorta, the iliac artery, and the femoral artery), renal artery stenosis caused by atherosclerosis or fibromuscular disease, superior vena cava syndrome, and occlusive iliac vein thrombosis resistant to thrombolysis.

5                   It is well recognized that one of the complications associated with endovascular techniques is the dislodgment of embolic materials generated during manipulation of the vessel, thereby causing occlusion of the narrower vessels downstream and ischemia or infarct of the organ which the vessel supplies. In 1995, Waksman et al. disclosed that distal embolization is common after directional  
10                   atherectomy in coronary arteries and saphenous vein grafts. See Waksman et al., American Heart Journal 129(3): 430-5 (1995), incorporated herein by reference. This study found that distal embolization occurs in 28% (31 out of 111) of the patients undergoing atherectomy. In January 1999, Jordan, Jr. et al. disclosed that treatment of carotid stenosis using percutaneous angioplasty with stenting is associated with more  
15                   than eight times the rate of microemboli seen using carotid endarterectomy. See Jordan, Jr, et al. Cardiovascular surgery 7(1): 33-8 (1999), incorporated herein by reference. Microemboli, as detected by transcranial Doppler monitoring in this study, have been shown to be a potential cause of stroke. The embolic materials include calcium, intimal debris, atheromatous plaque, thrombi, and/or air.

20                   There are a number of devices designed to provide blood filtering for entrapment of vascular emboli. The vast majority of these devices are designed for permanent placement in veins to prevent pulmonary embolism. A temporary venous filter device is disclosed in Bajaj, U.S. Patent No. 5,053,008 (this and all other references cited

herein are expressly incorporated by reference as if fully set forth in their entirety herein).

The Bajaj device is an intracardiac catheter for temporary placement in the pulmonary trunk of a patient predisposed to pulmonary embolism due to, *e.g.*, hip surgery, major trauma, major abdominal or pelvic surgery, or immobilization. The Bajaj device includes

5 an umbrella made from meshwork which traps venous emboli before they reach the lungs. This device is designed for venous filtration and is not suitable for arterial use because of the hemodynamic differences between arteries and veins.

There are very few intravascular devices designed for arterial use. Arteries are much more flexible and elastic than veins and, in the arteries, blood flow is pulsatile with large pressure variations between systolic and diastolic flow. These pressure variations cause the artery walls to expand and contract. Blood flow rates in the arteries vary from about 1 to about 5 L/min. Ginsburg, U.S. Patent No. 4,873,978, discloses an arterial filtering system, which includes a catheter with a strainer device at its distal end. This device is inserted into the vessel downstream from the treatment site and, after

10 treatment, the strainer is collapsed around the entrapped emboli and removed from the body. The Ginsburg device could not withstand flow rates of 5 L/min. It is designed for only small arteries and therefore could not capture emboli destined for all parts of the body. Ing. Walter Hengst GmbH & Co, German Patent DE 34 17 738, also discloses another arterial filter having a folding linkage system which converts the filter from the

15 collapsed to the expanded state.

20

Filters mounted to the distal end of guidewires have been proposed for intravascular blood filtration. A majority of these devices includes a filter which is attached to a guidewire and is mechanically actuated via struts or a pre-shaped basket

which deploys in the vessel. These filters are typically mesh "parachutes" which are attached to the shaft of the wire at the distal end and to wire struts which extend outward in a radial direction at their proximal end. The radial struts open the proximal end of the filter to the wall of the vessel. Blood flowing through the vessel is forced through the mesh thereby capturing embolic material in the filter. These devices are self-directing and can be placed intravascularly. However, one major disadvantage associated with the current devices is that the steerability of the guidewire may be altered as compared to the conventional guidewires due to the size of the filter. The guidewire may bend, kink, and/or loop around in the vessel, making insertion of the filter through a complex vascular lesion difficult.

During endovascular procedures, it is not uncommon to exchange one endovascular device for another over the guidewire. However, the guidewire position is often lost or compromised during the exchange of devices. For example, during coronary revascularization, it is often required to exchange of one guide catheter for another guide catheter possessing different qualities, *e.g.*, a larger diameter guide to deliver a specialized angioplasty device, a smaller diameter guide to prevent deep intubation and/or pressure damping, a different guide shape, or a guide catheter containing side holes. It is known that there are few interventional maneuvers as challenging as attempting to maintain distal guidewire access while trying to exchange one guiding catheter for another without compromising the guidewire position.

What is needed are simple and safe blood filtering and guidewire systems which can be temporarily placed in the arteries and veins to prevent distal embolization during endovascular procedures, and can be used to introduce and/or exchange various

instruments to a region of interest without compromising the position of the filter or guidewire. Existing devices are inadequate for this purpose.

#### Summary of the Invention

5           The present invention provides devices and methods for introduction of endovascular devices, *e.g.*, guide catheters, atherectomy catheters, angioplasty catheters, intravascular ultrasound catheters, or stent-deployment catheters, and for protecting a patient from distal embolization during cardiovascular procedures. More specifically, a guided filter system with support wire is disclosed for capturing embolic material  
10 generated during the procedure and for directing or exchanging other devices to a region of interest in an artery or vein.

          In one embodiment, the filter system comprises a guidewire and a support wire having an expandable filter, *e.g.*, a parachute, basket, or scroll, mounted on a distal region of the support wire. The support wire is adapted for percutaneous insertion into an  
15 artery or vein and is adapted to receive an endovascular instrument. The distal region of the support wire includes a wire guide, which slideably engages the guidewire. In certain embodiments, the wire guide comprises a ring having an aperture adapted to receive the guidewire.

          In another embodiment, the filter comprises an expansion frame and a  
20 mesh disposed over the frame. The filter can be placed in a collapsed condition to facilitate entry into a vessel and an enlarged condition to capture embolic material in the vessel. In certain embodiments, the frame comprises a plurality of struts bonded to the guidewire at a first end, and the struts expand radially outward at a second end. The



construction and use of expansion means and associated filter mesh have been thoroughly discussed in earlier applications including Barbut et al., U.S. Application Ser. No. 08/533,137, filed Nov. 7, 1995, Barbut et al., U.S. Application Ser. No. 08/580,223, filed Dec. 28, 1995, Barbut et al., U.S. Application Ser. No. 08/584,759, filed Jan 9, 1996, 5 Barbut et al., U.S. Application Ser. No. 08/640,015, filed Apr. 30 1996, Barbut et al., U.S. Application Ser. No. 08/645,762, filed May 14, 1996, and Barbut et al., U.S. Pat. No. 5,662,671, and the contents of each of these prior applications are expressly incorporated herein by reference.

The methods of the present invention include deployment of a  
10 percutaneous medical instrument during an endovascular procedure to remove plaque and/or thrombi from the coronary artery, aorta, common carotid artery, external and internal carotid arteries, brachiocephalic trunk, middle cerebral artery, basilar artery, subclavian artery, brachial artery, axillary artery, iliac artery, renal artery, femoral artery, popliteal artery, celiac artery, superior mesenteric artery, inferior mesenteric artery,  
15 anterior tibial artery, posterior tibial artery, and all other arteries carrying oxygenated blood. The methods also include prevention of distal embolization during an endovascular procedure to remove thrombi and/or foreign bodies in the venous circulation, including the superior vena cava, inferior vena cava, external and internal jugular veins, brachiocephalic vein, pulmonary artery, subclavian vein, brachial vein,  
20 axillary vein, iliac vein, renal vein, femoral vein, profunda femoris vein, great saphenous vein, portal vein, splenic vein, hepatic vein, and azygous vein.

In a first method of using the guided filter system, the distal end of the guidewire is inserted percutaneously through an artery or vein and advanced into or

beyond a region of interest, typically a stenotic lesion caused by buildup of atherosclerotic plaque and/or thrombi. In a collapsed condition, the filter and the distal region of the support wire are advanced over the guidewire, having the wire guide of the support wire engaging the guidewire, *i.e.*, like a monorail catheter engaging a guidewire.

- 5 The filter is expanded downstream of the vascular occlusion, and the guidewire is withdrawn and removed from the body. The distal region of an endovascular device, such as an atherectomy, stent-deployment, or angioplasty catheter, is inserted over the support wire and advanced to the region of interest. After the stenotic lesion is removed or otherwise treated by the endovascular device and an adequate luminal diameter is
- 10 established, the filter is collapsed and removed, together with the captured embolic debris, from the vessel by withdrawing the support wire.

- In another method, after the guidewire and the support wire with the expanded filter are positioned in a vessel distal to the region of interest, the endovascular device is inserted over both the guidewire and the support wire to position within the
- 15 region of interest. During certain cardiovascular procedures, especially coronary revascularization, exchange of endovascular instruments and catheters is needed and is difficult to accomplish because the initial guidewire positioning across the region of interest is often lost as the first device is withdrawn. Using the guided filter system, the guidewire and the support wire are both advanced distal to the region of interest. If the
- 20 position of the guidewire is lost during the withdrawal of the first device, the second device that needs to be exchanged can be advanced over the support wire to be positioned within the region of interest.

It will be understood that there are several advantages in using the devices

and methods disclosed herein for capturing and removing embolic debris during endovascular procedures. For example, the guided filter system (1) is particularly well suited for temporary filtration of blood in any vessel to entrap embolic debris, thereby minimizing neurologic, cognitive, and cardiac complications associated with distal embolization, (2) can withstand high arterial blood flow for an extended time, (3) includes a mesh that is sufficiently porous to allow adequate blood flow in a blood vessel while capturing emboli, (4) can be used to direct an endovascular catheter to a region of interest in the vessel, (5) can be used to exchange medical instruments without compromising the position of the guidewire, and (6) can be used in adult and pediatric patients.

#### Brief Description of the Drawings

Fig. 1A depicts an embodiment of a support wire having a filter in a collapsed condition according to the present invention.

Fig. 1B depicts the support wire of Fig. 1A having the filter in an expanded condition.

Fig. 1C depicts a cross-sectional view through section line C – C of the support wire depicted in Fig. 1B.

Fig. 1D depicts the support wire of Fig. 1C having a guidewire received through the wire guide mounted within the filter.

Fig. 1E depicts the support wire of Fig. 1C having a guidewire received through the wire guide mounted proximal to the filter.

Fig. 1F depicts the support wire of Fig. 1C having a guidewire received

through the wire guide mounted distal to the filter.

Fig. 1G depicts the guidewire and the support wire carried within a rapid exchange catheter.

Fig. 1H depicts the catheter of Fig. 1G deployed over an atheromatous lesion in a vessel.

Fig. 1I depicts the guidewire and the support wire carried within a rapid exchange catheter.

Fig. 1J depicts the guidewire and the support wire carried within a rapid exchange catheter.

Fig. 1K depicts the guidewire and the support wire carried within a rapid exchange catheter.

Fig. 2A depicts an embodiment of a distal end of the guidewire.

Fig. 2B depicts an alternative embodiment of the distal end of the guidewire.

Fig. 2C depicts another alternative embodiment of the distal end of the guidewire.

Fig. 3A depicts another embodiment of the filter shaped as a parachute,

Fig. 3B depicts another embodiment of the filter shaped as an eggbeater.

Fig. 4A depicts a guidewire inserted across a vascular occlusion.

Fig. 4B depicts the filter and support wire engaging the guidewire with the filter expanded beyond the vascular occlusion.

Fig. 4C depicts an angioplasty catheter inserted over the support wire.

Fig. 4D depicts an angioplasty catheter inserted over the guidewire and the

support wire.

#### Detailed Description

In a first embodiment, a filter system for temporary placement in a vessel,  
5 either an artery or vein, is provided as depicted in Figs. 1A, 1B, 1C, and 1D. The filter  
system includes support wire 10 having a proximal end, distal region 11, and expandable  
filter 20 mounted at the distal region. The filter comprises expansion frame 22 and mesh  
25 which is sonic welded or adhesive bonded to struts 28 of the expansion frame.  
Anticoagulants, such as heparin and heparinoids, may be applied to mesh 25 to reduce  
10 thrombi formation on the mesh. The filter can be collapsed as shown in Fig. 1A to  
facilitate insertion into a vessel, and thereafter expanded as shown in Fig. 1B. Wire guide  
26 is included in distal region 11 of the support wire. The wire guide may be mounted  
within the filter (as shown in Fig. 1B and Fig. 1C) or at any other suitable position on  
support wire 10 proximal of the filter (as shown in Fig. 1E), or on a distal extension of  
15 the support wire which extends beyond the filter (as shown in Fig. 1F). In certain  
embodiments, the support wire may comprise a ring. A cross-sectional view of the  
support wire through section line C – C is depicted in Fig. 1C. The design and  
construction of a variety of filters for use on guidewire is described in detail in Tsugita et  
al., U.S. Patent No. 5,911,734, the disclosure of which is expressly incorporated herein  
20 by reference in its entirety.

In another embodiment, the filter further includes a capture sheath which  
covers the filter and is removeable from the filter, the sheath having a port in its distal  
region adapted to receive the guidewire in the manner of a rapid exchange catheter. In

Fig. 1G, support wire 10 is inserted in lumen 51 of a rapid exchange catheter 50. The catheter includes side port 60 in its distal region, adapted to receive guidewire 30. In Fig. 1I, the catheter includes skive 61 which receives guidewire 30. In Fig. 1J, elongate member 70 carries tubular segment 75 having skive 77 at a distal region of elongate member 70. The tubular segment acts as a capture sheath for the filter while the skive receives the guidewire. In Fig. 1K, elongate member 70 carries first and second tubular segments, 75 and 79, adapted to receive, respectively, the filter and the guidewire.

When in use, guidewire 30 is first inserted into a vessel and advanced distal to the region of interest. The catheter, which carries the filter in lumen 51, is inserted over the guidewire, the guidewire engaged through side port 60. The filter is advanced distally passing atheromatous lesion 100. The guidewire can then be withdrawn and catheter 50 drawn proximal, leaving the catheter and the filter inserted in the vessel as depicted in Fig. 1H. Catheter 50 is then removed from the vessel.

Expansion frame 22 is expanded to capture embolic materials downstream the atheromatous lesion. An endovascular device, such as an angioplasty catheter with or without a stent, can be inserted over support wire 10 to position adjacent atheroma 100. After vascular procedures are performed with the endovascular device(s), the device(s) are withdrawn and removed from the vessel. The filter with the captured emboli is then contracted and removed.

The filter system also includes guidewire 30 having a proximal end and distal end 33. The guidewire is slideably received by support wire 10 through wire guide 26 as depicted in Fig. 1D. The filter system further includes endovascular devices, such as atherectomy catheters, endovascular imaging devices, stent-deployment catheters,

angioplasty catheters, pressure monitors, electrophysiology catheters, and aspirators, which are adapted to receive guidewire 30 and/or support wire 10 in their lumens.

Different constructions of distal end 33 of the guidewire are depicted in Figs. 2A, 2B, and 2C. Distal end 33 may assume a substantially linear configuration relative to the proximal end of the guidewire as depicted in Fig. 2A. Alternatively, distal end 33 may assume an angular configuration relative to the proximal end of the guidewire as depicted in Fig. 2A. Distal end 33 may be shaped like a fishhook as depicted in Fig. 2C. The distal region of the guidewire may be constructed of a flexible material to facilitate entry through a region of interest, and preferably is equipped with an atraumatic tip as is known in the art. The embodiments in Figs. 2B and 2C, having a curvilinear design, are particularly useful in achieving access to a complex lesion in a tortuous vessel.

Figs. 3A and 3B depict alternative embodiments of expandable filter 20 mounted on the distal region of support wire 10. In Fig. 3A, filter 20 comprises a parachute frame, and mesh 25 which is welded (e.g., sonic or laser) or adhesive bonded to struts 28. Wire guide 26 is included in the distal region of the support wire and projects distally from filter 20 for engaging a guidewire. In Fig. 3B, filter 20 comprises compressible struts 22, and mesh 25. In an expanded condition, filter 20 assumes the shape of an eggbeater.

By way of example, when the filter system as disclosed herein is intended for use in the aorta, the area of the mesh required for the device is calculated from Bernoulli's equation as described in our earlier applications including Barbut et al., U.S. Application Serial No., U.S. Application Serial No. 08/553,137, filed November 7, 1995,

Barbut et al., U.S. Application Serial No. 08/580,223, filed December 28, 1995, Barbut et al., U.S. Application Serial No. 08/584,759, filed January 9, 1996, Barbut et al., U.S. Application Serial No. 08/640,015, filed April 30, 1996, and Barbut et al., and U.S. Application Serial No. 08/645,762, filed May 14, 1996, all of which are incorporated  
5 herein by reference.

In an embodiment of the guided filter system that is to be used in the aorta, mesh with dimensions within the following ranges is desirable: mesh area is  $0.004\text{--}5\text{ in}^2$ , more preferably  $0.007\text{--}4\text{ in}^2$ , more preferably  $0.010\text{--}3\text{ in}^2$ , more preferably  $0.015\text{--}2\text{ in}^2$ , more preferably  $0.020\text{--}1\text{ in}^2$ , more preferably  $0.025\text{--}0.076\text{ in}^2$ ; mesh thickness is  $60\text{--}280$   
10  $\mu\text{m}$ , more preferably  $70\text{--}270\text{ }\mu\text{m}$ , more preferably  $80\text{--}260\text{ }\mu\text{m}$ , more preferably  $90\text{--}250\text{ }\mu\text{m}$ , more preferably  $100\text{--}250\text{ }\mu\text{m}$ , more preferably  $120\text{--}230\text{ }\mu\text{m}$ , more preferably  $140\text{--}210\text{ }\mu\text{m}$ ; thread diameter is  $30\text{--}145\text{ }\mu\text{m}$ , more preferably  $40\text{--}135\text{ }\mu\text{m}$ , more preferably  $50\text{--}125\text{ }\mu\text{m}$ , more preferably  $60\text{--}115\text{ }\mu\text{m}$ , more preferably  $70\text{--}105\text{ }\mu\text{m}$ , and pore size is  $500\text{ }\mu\text{m}$  or less, more preferably  $400\text{ }\mu\text{m}$  or less, more preferably  $300\text{ }\mu\text{m}$  or less, more  
15 preferably  $200\text{ }\mu\text{m}$  or less, more preferably  $100\text{ }\mu\text{m}$  or less, more preferably  $50\text{ }\mu\text{m}$  or less and usually larger than at least a red blood cell. In a preferred embodiment of the invention, mesh area is  $2\text{--}8\text{ in}^2$ , mesh thickness is  $60\text{--}200\text{ }\mu\text{m}$ , thread diameter is  $30\text{--}100\text{ }\mu\text{m}$ , and pore size is  $50\text{--}300\text{ }\mu\text{m}$ . In a further preferred embodiment of the invention, mesh area is  $3\text{--}5\text{ in}^2$ , mesh thickness is  $60\text{--}150\text{ }\mu\text{m}$ , thread diameter is  $50\text{--}80\text{ }\mu\text{m}$ , and  
20 pore size is  $100\text{--}250\text{ }\mu\text{m}$ . In other embodiments, the filter comprises a thin film laser cut with holes to allow blood flow. Typical dimensions include pore size of  $20\text{--}500\text{ }\mu\text{m}$ , a thickness of  $0.0005\text{--}0.003$  inches, and area approximately same as for meshes described



above.

In other embodiments, the filter comprises a thin film laser cut with holes to allow blood flow. Typical dimensions include pore size of 20-500  $\mu\text{m}$ , a thickness of 0.0005-0.003 inches, and area approximately same as for meshes described above .

5           Once appropriate physical characteristics are determined, suitable mesh can be found among standard meshes known in the art. For example, polyester meshes may be used, such as meshes made by Saati Corporations and Tetko Inc. These are available in sheet form and can be easily cut and formed into a desired shape. In a preferred embodiment, the mesh is welded (*e.g.* sonic or laser) or sewn into a cone shape.

10   Other meshes known in the art, which have the desired physical characteristics, are also suitable. Anticoagulants, such as heparin and heparinoids, may be applied to the mesh to reduce the chances of blood clotting on the mesh. Anticoagulants other than heparinoids also may be used, *e.g.*, monoclonal antibodies such as ReoPro (Centocor). The anticoagulant may be painted or sprayed onto the mesh. A chemical dip comprising the

15   anticoagulant also may be used. Other methods known in the art for applying chemicals to mesh may be used.

In use, as depicted in Fig. 4A, guidewire 30 is inserted percutaneously through a peripheral artery or vein and advanced typically in the direction of blood flow. However, guidewire 30 may be inserted and advanced in a direction opposite the blood

20   flow, *e.g.*, retrograde through the descending aorta to reach the coronary artery. Distal end 33 of the guidewire is passed through occluding lesion 100, typically an atheromatous plaque, and positioned distal to the occlusion. Support wire 10 of Fig. 1A

is inserted over the proximal end of guidewire 30 through wire guide 26, and advanced distally until filter 20 is positioned distal to plaque 100 as depicted in Fig. 4B. By having wire guide 26 engage the guidewire, the filter and the support wire can be easily steered intravascularly to reach the region of interest. Filter 20 is expanded to capture embolic material, such as calcium, thrombi, plaque, and/or tissue debris. Guidewire 30 is then withdrawn, leaving support wire 10 in position to direct an endovascular device to plaque 100.

Percutaneous transluminal angioplasty has been successful in treating arterial stenoses as well as occlusive venous thrombosis resistant to thrombolysis. See American Heart Journal, 125 (2 Pt 1): 362-6 (1993). Angioplasty catheter 40, which has angioplasty balloon 42 mounted on the distal region, is inserted over support wire 10 as depicted in Fig. 4C. In a deflated state, the angioplasty balloon is advanced over support wire 10 to a position adjacent plaque 100. The atheromatous plaque is compressed by inflating balloon 42, thereby dilating the stenosis in the vessel. In certain embodiments, the angioplasty catheter includes infusion port 44 proximal and perfusion port 45 distal to balloon 42. Infusion port 44 may be used to administer pharmaceutical agents, e.g., t-PA, adenosine, or nitroglycerin through the catheter lumen (not shown). Oxygenated medium or blood may be infused through port 45 to maintain perfusion to distal organs during angioplasty. In certain embodiments, a stent is closely associated with the angioplasty balloon. The stent is typically crimped onto the balloon and is capable of controlled radial expansion in the region of interest upon application of a radial, outwardly extending force from the interior of the stent. The construction of the catheter system carrying a stent is described in detail in Jang et al., U.S. Pat. No. 5,749,848, which

is incorporated herein by reference in its entirety.

The angioplasty catheter or other endovascular instrument is withdrawn from the vessel after completion of angioplasty. Embolic material generated during the angioplasty is captured and retained by filter 20. The filter is then contracted, and with  
5 captured embolic material, is withdrawn from the vessel and removed from the patient's body.

Alternatively, after filter 20 is positioned and expanded distal to plaque 100, guidewire 30 and support wire 10 may remain in the vessel across plaque 100 as depicted in Fig. 4D. Angioplasty catheter 40 is then inserted over both guidewire 30 and  
10 support wire 10 to a position adjacent plaque 100. If an atherectomy device, for example, is required to remove plaque remaining after angioplasty, angioplasty catheter 40 is withdrawn, with or without the guidewire, and an atherectomy catheter is inserted over guidewire 30 and/or support wire 10 to a position adjacent the plaque. In this way, if the position of guidewire 30 across the plaque is lost during the removal of angioplasty  
15 catheter 40, support wire 10 is available to direct another endovascular device to the region of interest. This method is particularly useful for exchanging guide catheters during coronary revascularization.

The length of the guidewire and the support wire will generally be between 30 and 300 centimeters, preferably approximately between 50 and 180  
20 centimeters. The filter will be capable of expanding to an outer diameter of at least 0.2 centimeters, more preferably at least 0.5 centimeters, more preferably at least 1.0 centimeters, more preferably at least 1.5 centimeters, more preferably at least 2.0 centimeters, more preferably at least 2.5 centimeters, more preferably at least 3.0

centimeters, more preferably at least 3.5 centimeters, more preferably at least 4.0 centimeters, more preferably at least 4.5 centimeters, more preferably at least 5.0 centimeters. These ranges cover suitable diameters for both pediatric and adult use. The foregoing ranges are set forth solely for the purpose of illustrating typical device

5 dimensions. The actual dimensions of a device constructed according to the principles of the present invention may obviously vary outside of the listed ranges without departing from those basic principles.

Although the foregoing invention has, for the purposes of clarity and understanding, been described in some detail by way of illustration and example, it will

10 be obvious that certain changes and modifications may be practiced which will still fall within the scope of the appended claims. Moreover, it will be understood that each and every feature described for any given embodiment or in any reference incorporated herein, can be combined with any of the other embodiments described herein.

What is claimed is:

1. A method for deploying a percutaneous medical instrument,  
comprising the steps of:  
providing a guidewire and a support wire, the support wire having a distal  
5 region, a wire guide mounted on the distal region, and an expandable filter mounted on  
the distal region;  
advancing the guidewire into a region of interest within a vessel;  
advancing the support wire along the guidewire with the wire guide of the  
support wire engaging the guidewire;  
10 expanding the filter downstream of the region of interest; and  
advancing the percutaneous medical instrument over the support wire and  
positioning the medical instrument within the region of interest.
2. The method of claim 1, further comprising the step of removing  
the guidewire from the vessel.
- 15 3. The method of claim 1, wherein the region of interest is within a  
coronary artery.
4. The method of claim 1, wherein the region of interest is within a  
carotid artery.

5. The method of claim 1, wherein the region of interest contains atheromatous plaque.

6. The method of claim 1, wherein the wire guide comprises a ring having an aperture adapted to receive the guidewire.

5 7. The method of claim 1, wherein the percutaneous medical instrument is an angioplasty catheter.

8. The method of claim 1, wherein the percutaneous medical instrument is a stent-deployment catheter.

9. The method of claim 8, wherein the stent-deployment catheter  
10 comprises a sheath disposed about a self-expanding stent.

10. The method of claim 1, wherein the percutaneous medical instrument is an atherectomy catheter.

11. The method of claim 1, wherein the percutaneous medical instrument is an aspiration catheter.

15 12. The method of claim 7, further comprising the step of inflating the angioplasty balloon at the region of interest, wherein embolic material is captured by the filter.

13. The method of claim 8, further comprising the step of expanding the stent at the region of interest, wherein embolic material is captured by the filter.
14. The method of claim 1, further comprising the step of:  
contracting the filter; and  
5 removing the support wire from the vessel.
15. The method of claim 1, further comprising the step of removing the percutaneous medical instrument from the vessel.
16. The method of claim 1, wherein the expandable filter comprises a plurality of struts and a mesh disposed about the struts.
- 10 17. The method of claim 1, wherein the filter expands to the shape of an eggbeater.
18. The method of claim 1, further comprising the step of exchanging one percutaneous medical instrument for another.

19. A percutaneous filter system, comprising:  
a guidewire;  
a support wire having a proximal end, a distal end, and a distal region, the support wire adapted to receive a percutaneous medical instrument;  
5 an expandable filter mounted on the distal region of the support wire; and  
a wire guide mounted on the distal region of the support wire and  
slideably engaging the guidewire,  
wherein, during use, the guidewire is positioned in a vessel at a region of interest, and the support wire is advanced along the guidewire until the filter reaches the  
10 region of interest.
20. The system of claim 19, wherein the expandable filter is manually activated.
21. The system of claim 19, wherein the expandable filter is self-  
15 activating.
22. The system of claim 19, wherein the wire guide comprises a ring having an aperture adapted to receive the guidewire.
23. The system of claim 19, wherein the expandable filter comprises a plurality of struts and a mesh disposed about the struts.



24. The system of claim 23, wherein the mesh is woven.
25. The system of claim 23, wherein the mesh is a thin film having  
holes to allow fluid flow.
26. The system of claim 19, wherein the filter expands to the shape of  
5 an eggbeater.
27. The system of claim 19, further comprising a percutaneous medical  
instrument selected from the group consisting of an angioplasty catheter, a stent-  
deployment catheter, an atherectomy catheter, intravascular ultrasound catheter, and an  
aspiration catheter.
- 10 28. The system of claim 27, wherein the stent-deployment catheter  
comprises a sheath disposed about a self-expanding stent.
29. The method of claim 1, wherein the wire guide is mounted on the  
support wire within the filter.
30. The method of claim 1, wherein the wire guide is mounted on the  
15 support wire distal the filter.

31. A percutaneous filter system, comprising:  
a guidewire;  
a support wire having a proximal end, a distal end, a distal region, and an expandable filter mounted on the distal region of the support wire, the support wire  
5 adapted to receive a percutaneous medical instrument; and  
a sheath which removeably covers the support wire and filter, the sheath having a proximal end, a distal end, and a distal region, the distal region having a lumen which receives the filter and an aperture adapted to pass the guidewire,  
wherein, during use, the guidewire is positioned in a vessel at a region of  
10 interest, the sheath carrying the support wire is advanced along the guidewire until the filter reaches the region of interest, and the sheath is withdrawn to expose the filter.
32. The filter system of claim 31, wherein the lumen of the sheath extends from the distal region to the proximal end.
33. The filter system of claim 31, wherein the sheath comprises an  
15 elongate member having a cylindrical segment at a distal end of the elongate member, wherein the distal region of the sheath comprises the cylindrical segment.
34. The filter system of claim 31, wherein the aperture communicates with the lumen of the sheath.

35. A method for deploying a percutaneous medical instrument,  
comprising the steps of:

- providing a guidewire, a support wire, and a sheath, the support wire  
having an expandable filter mounted on the distal region, the sheath covering the  
5 expandable filter;  
advancing the guidewire into a region of interest within a vessel;  
advancing the sheath and the support wire along the guidewire with the  
sheath engaging the guidewire;  
withdrawing the sheath from the expandable filter;  
10 expanding the filter downstream of the region of interest; and  
advancing the percutaneous medical instrument over the support wire and  
positioning the medical instrument within the region of interest.

36. The method of claim 35, wherein the sheath engages the guidewire  
through an aperture in a distal region of the sheath.

- 15 37. The method of claim 35, wherein the step of withdrawing the  
sheath from the expandable filter comprises retracting the sheath proximally.

38. The method of claim 35, wherein the step of withdrawing the  
sheath from the expandable filter comprises advancing the sheath distally.

39. The method of claim 35, further comprising the step of removing the sheath from the vessel.

40. The method of claim 31, wherein the aperture is located 10cm from the distal end of the sheath.

5

10

1 / 7

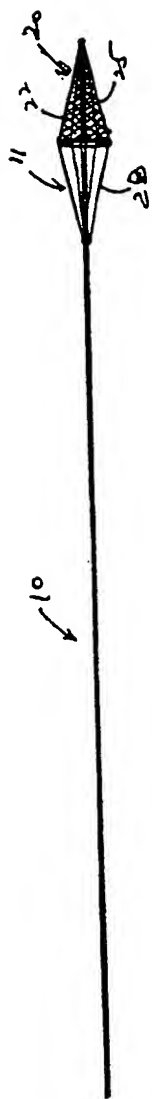


FIG. 1A




FIG. 1C

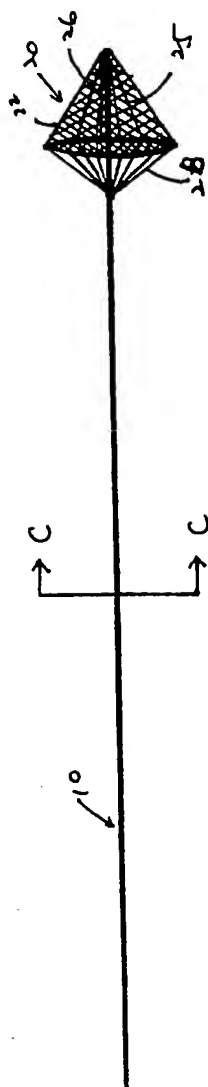


FIG. 1B

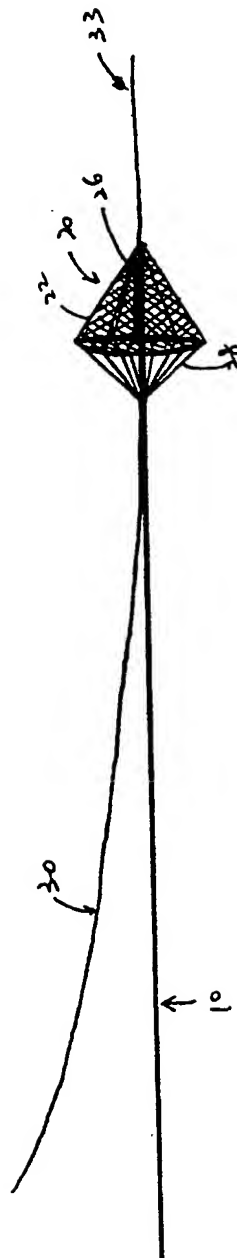


FIG. 1D



FIG. 1E



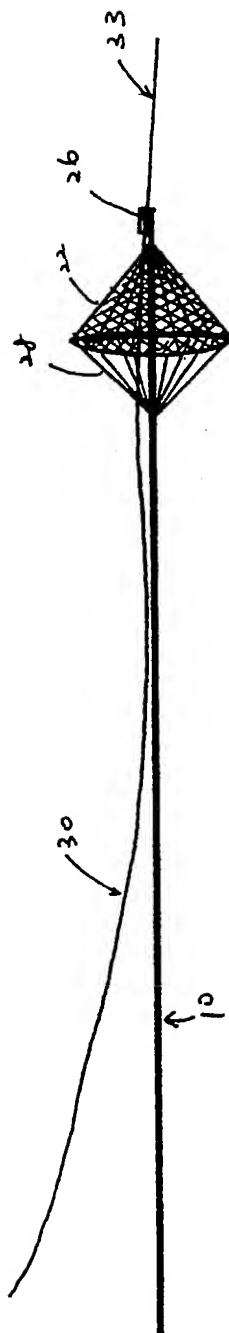


FIG. 1F


3 / 7

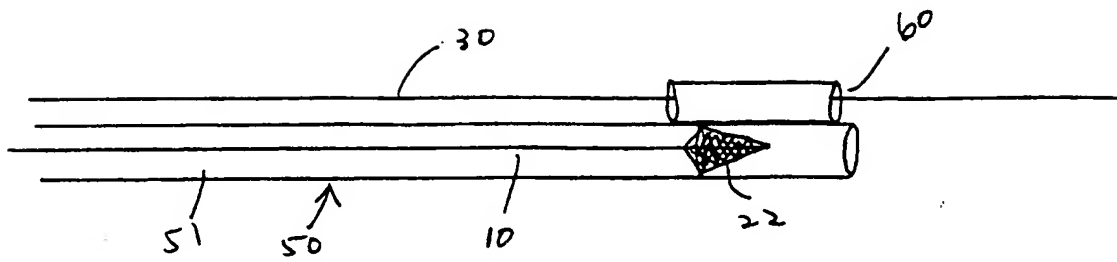


**FIG. 1G**

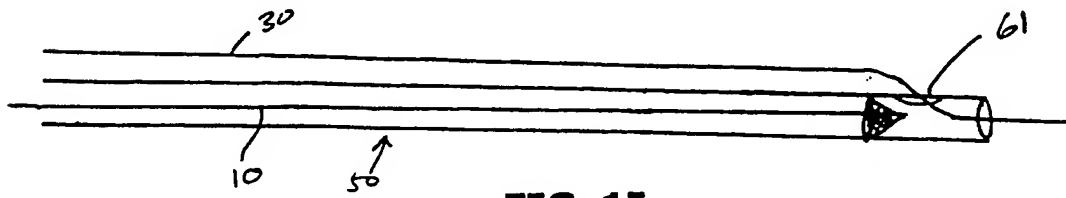


**FIG. 1I**

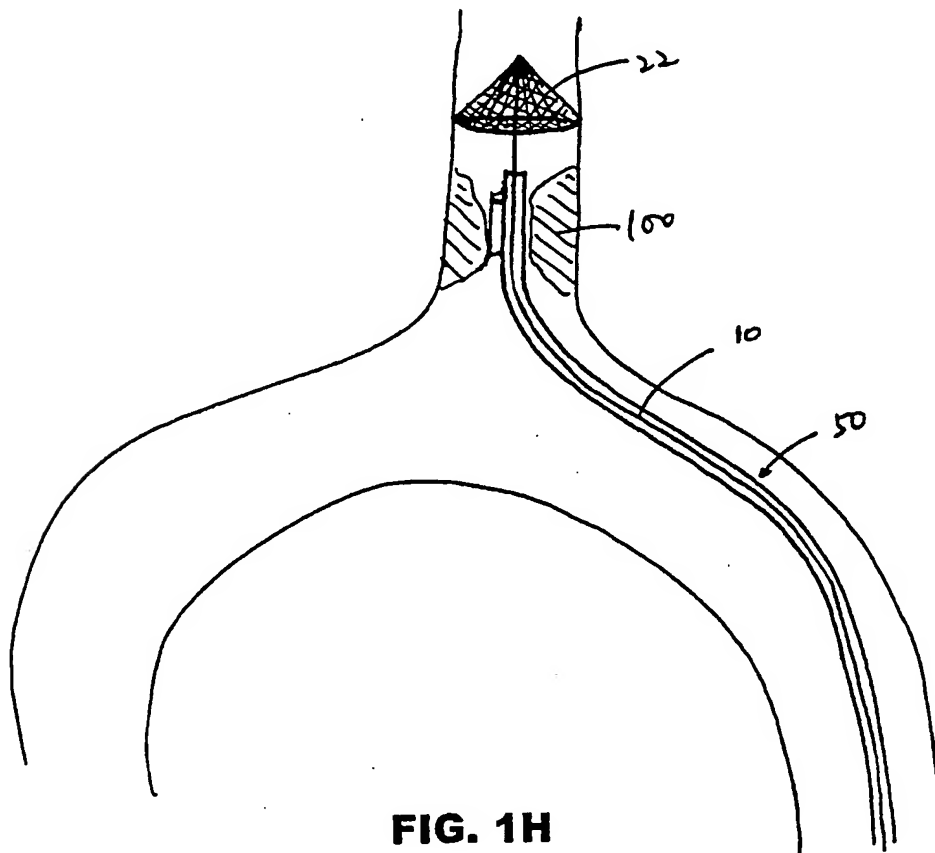

**FIG. 1H**

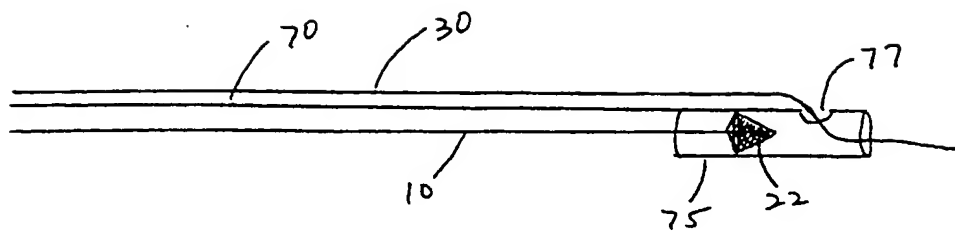

**FIG. 1J**

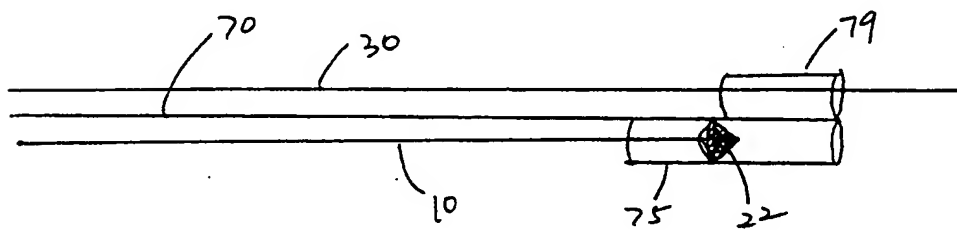

**FIG. 1K**



5 / 7



FIG. 2A



FIG. 2B



FIG. 2C

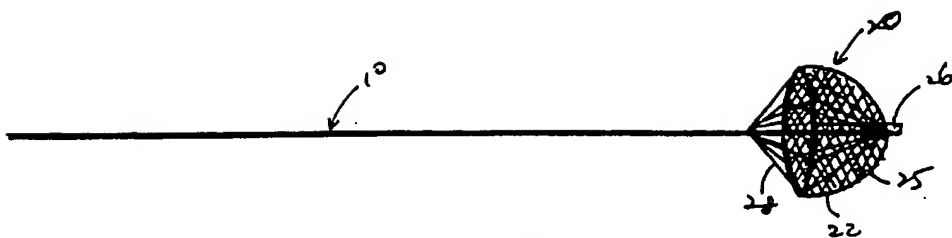


FIG. 3A



FIG. 3B

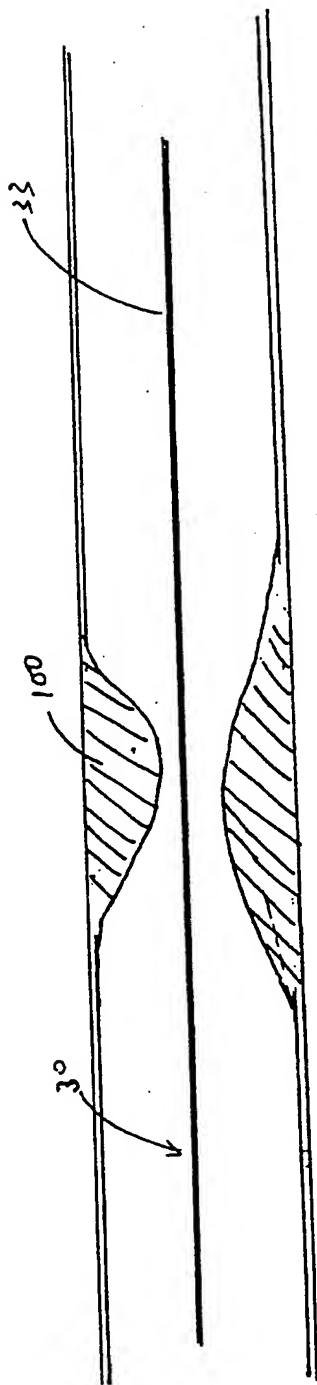


FIG. 4A

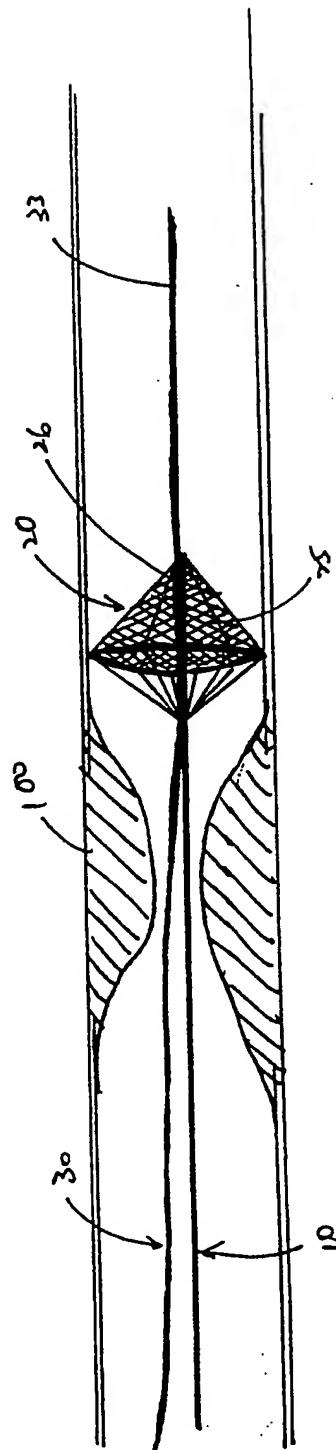


FIG. 4B

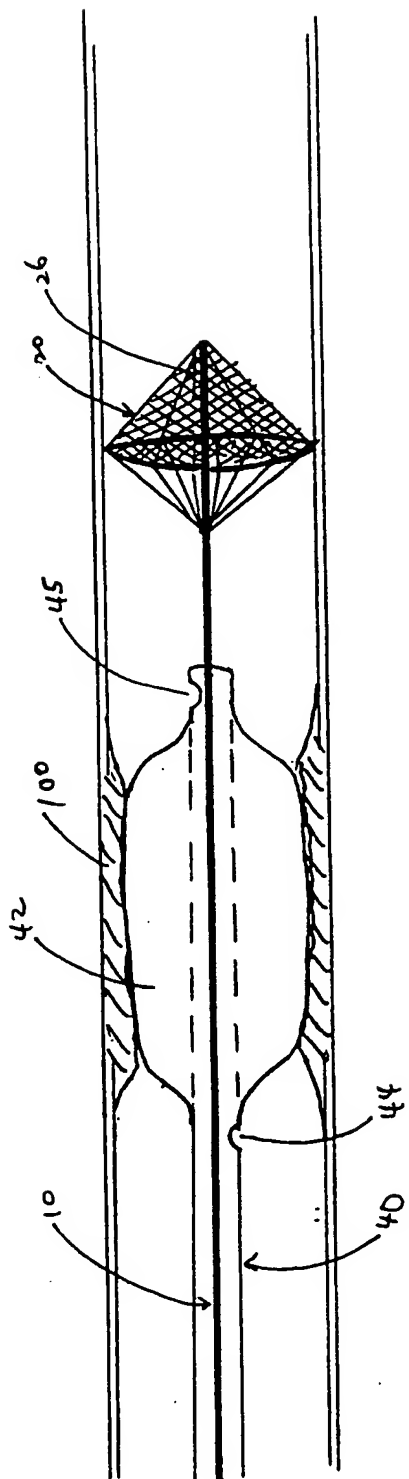


FIG. 4C

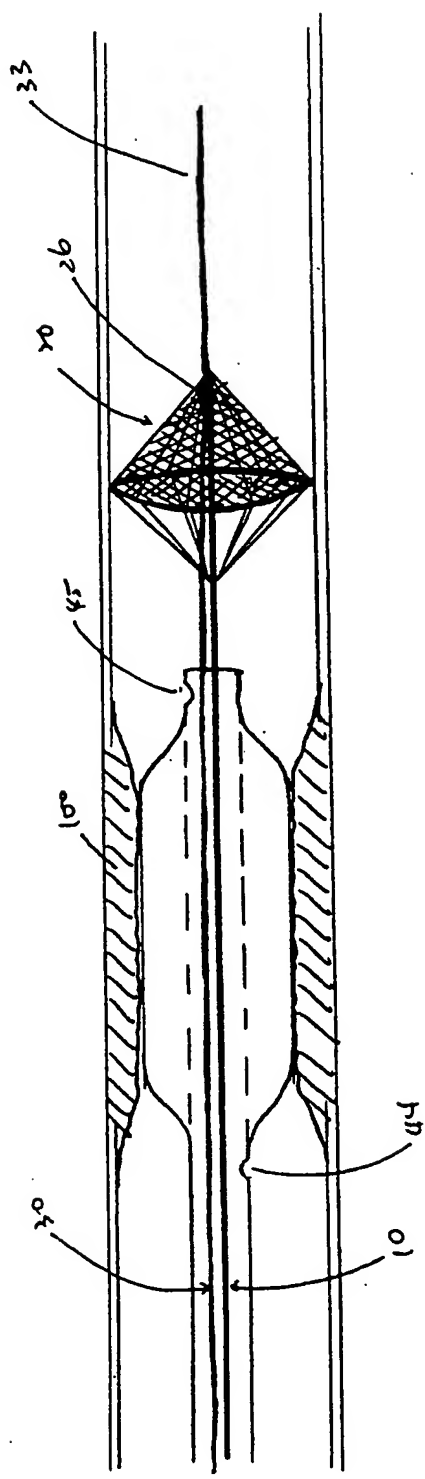


FIG. 4D

# INTERNATIONAL SEARCH REPORT

International Application No  
PCT/US 00/40559

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61F2/01

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)  
IPC 7 A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 98 33443 A (YADAV JAY S ;ANGIOGUARD INC (US)) 6 August 1998 (1998-08-06) figure 7 page 10, line 29 -page 11, line 30	19,31
A	US 4 723 549 A (WHOLEY MARK H ET AL) 9 February 1988 (1988-02-09) figures 1-3 column 2, line 62 -column 3, line 39	19,31
A	FR 2 666 980 A (LG MEDICAL ;PIERONNE ALAIN (FR)) 27 March 1992 (1992-03-27) figures 1-4 page 8, line 34 -page 11, line 27 --- -/--	19,31

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents :

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \*&\* document member of the same patent family

Date of the actual completion of the international search

6 December 2000

Date of mailing of the international search report

13/12/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Mary, C

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 00/40559

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 848 964 A (SAMUELS SHAUN LAWRENCE WILKIE) 15 December 1998 (1998-12-15) figures 1-4C column 3, line 54 - line 60 column 4, line 13 - line 25 claims 1-4	19,31
A	US 4 643 184 A (MOBIN-UDDIN KAZI) 17 February 1987 (1987-02-17) figures 12-23 column 4, line 56 -column 5, line 54	19,31

# INTERNATIONAL SEARCH REPORT

information on patent family members

International Application No

PCT/US 00/40559

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9833443	A	06-08-1998	AU 6052798 A CA 2250777 A EP 0938276 A JP 2000504263 T	25-08-1998 06-08-1998 01-09-1999 11-04-2000
US 4723549	A	09-02-1988	NONE	
FR 2666980	A	27-03-1992	NONE	
US 5848964	A	15-12-1998	WO 9855175 A US 5947995 A	10-12-1998 07-09-1999
US 4643184	A	17-02-1987	US 4727873 A	01-03-1988